

EINGEGANGEN
03 Juli 2013
TQM

[Handwritten signature]

International proficiency testing scheme - Ciclosporin

Centre 145



PT Distribution 351



Samples dispatched on: 4th June 2013

Results deadline: 28th June 2013

Method: ACMA – on Dimension platform

Group Code: ACMA

Bias plot: Distribution 348 - 351

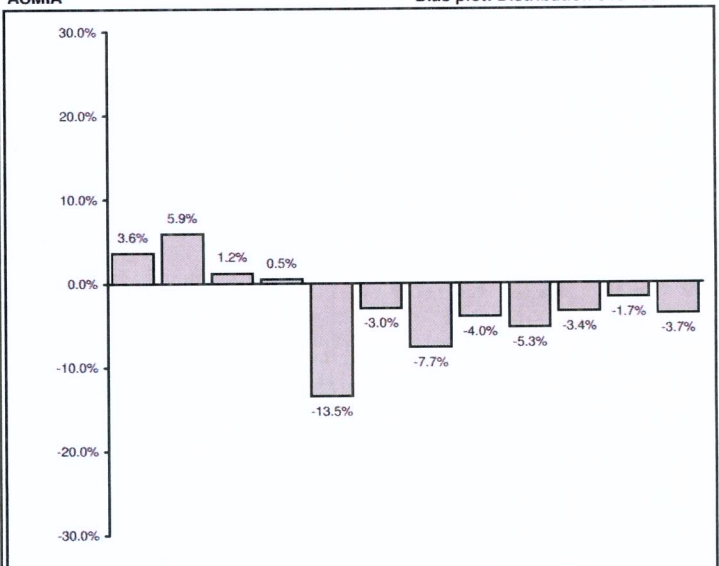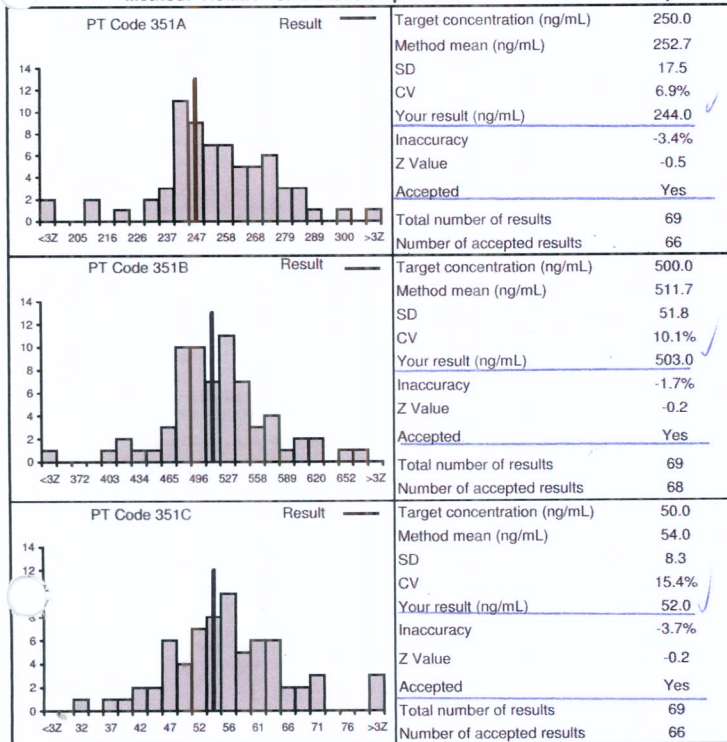

PT Code	348A	348B	348C	349A	349B	349C	350A	350B	350C	351A	351B	351C
Bias	3.6%	5.9%	1.2%	0.5%	-13.5%	-3.0%	-7.7%	-4.0%	-5.3%	-3.4%	-1.7%	-3.7%
Target value	Pool	Pool	Pool	250.0	800.0	50.0	Pool	250.0	100.0	250.0	500.0	50.0
Method Mean	122.6	122.8	115.6	227.9	793.1	47.4	169.1	238.5	101.4	252.7	511.7	54.0
Your value	127.0	130.0	117.0	229.0	686.0	46.0	156.0	229.0	96.0	244.0	503.0	52.0
Accepted	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes

[Handwritten signature]