

Centre 1022

PT Distribution 212

Samples dispatched on: 8th January 2013

Results deadline: 1st February 2013


EINGEGANGEN
06. Feb. 2013
TQM

TACROLIMUS
International Proficiency
Testing Scheme


Method: CMIA - on Architect platform

Group Code: Architect


Bias plot: Distribution 209 - 212

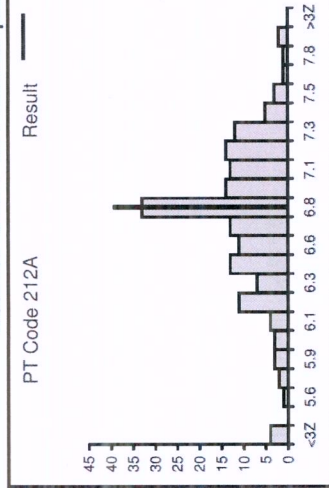


Target concentration (ng/mL)	Pool
Method mean (ng/mL)	6.7
SD	0.4
CV	6.0%
Your result (ng/mL)	6.8 ✓
Inaccuracy	+1.5%
Z Value	0.2
Accepted	Yes ✓
Total number of results	170
Number of accepted results	166

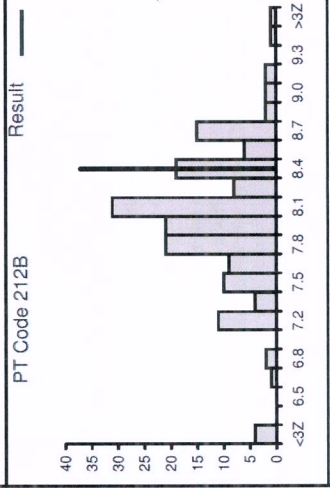

Target concentration (ng/mL)	Pool
Method mean (ng/mL)	7.9
SD	0.5
CV	6.3%
Your result (ng/mL)	8.3 ✓
Inaccuracy	+5.1%
Z Value	0.8
Accepted	Yes
Total number of results	170
Number of accepted results	165

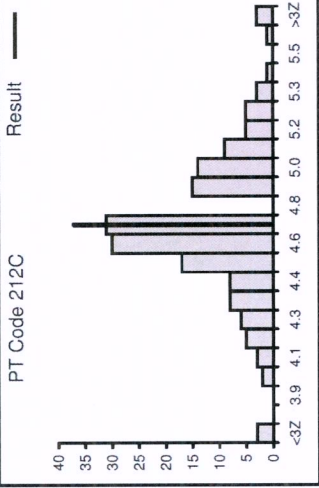

Target concentration (ng/mL)	Pool
Method mean (ng/mL)	4.7
SD	0.3
CV	6.4%
Your result (ng/mL)	4.7 ✓
Inaccuracy	+0.0%
Z Value	0.0
Accepted	Yes
Total number of results	170
Number of accepted results	162

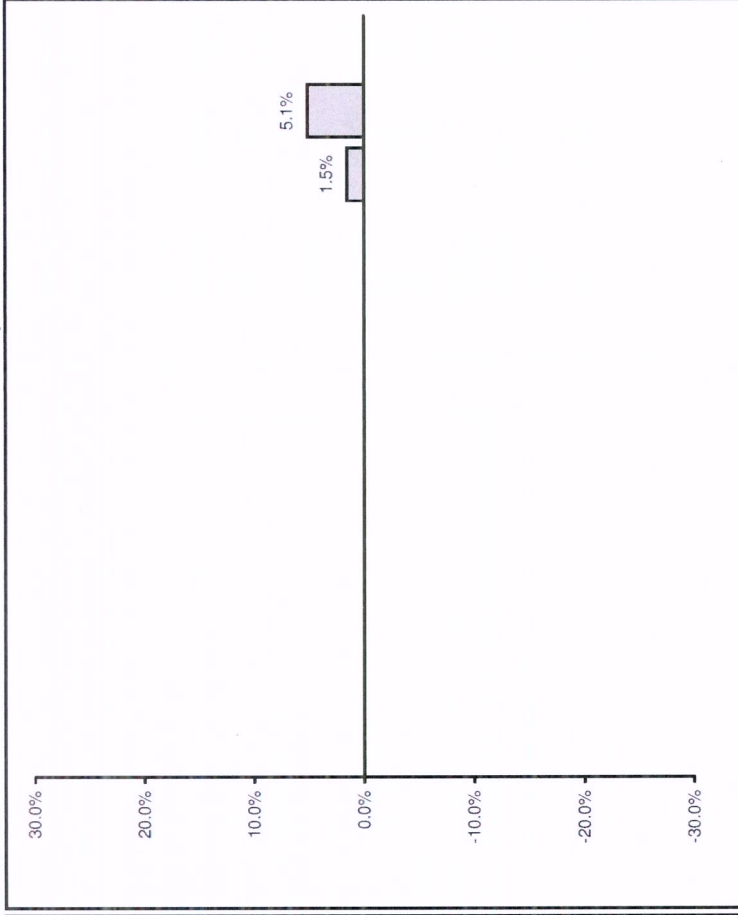

PT Code	209A	209B	209C	210A	210B	210C	211A	211B	211C	212A	212B	212C
Bias										1.5%	5.1%	0.0%
Target value	18.0	4.0	9.0	12.0	Pool	4.0	8.0	20.0	Pool	Pool	Pool	Pool
Method Mean	17.4	3.9	9.4	12.7	10.0	4.3	8.4	19.7	10.0	6.7	7.9	4.7
Your value										6.8	8.3	4.7
Accepted										Yes	Yes	Yes

