


Centre 1022

PT Distribution 241

Samples dispatched on: 02 June 2015





Results deadline: 26 June 2015

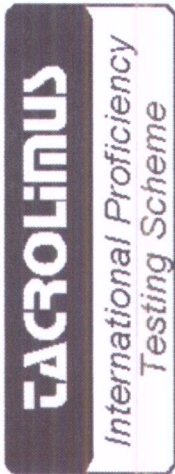

Method: HPLC/MS or HPLC/MS/MS

Group Code: HPLC/MS

Bias plot: Distribution 238 - 241

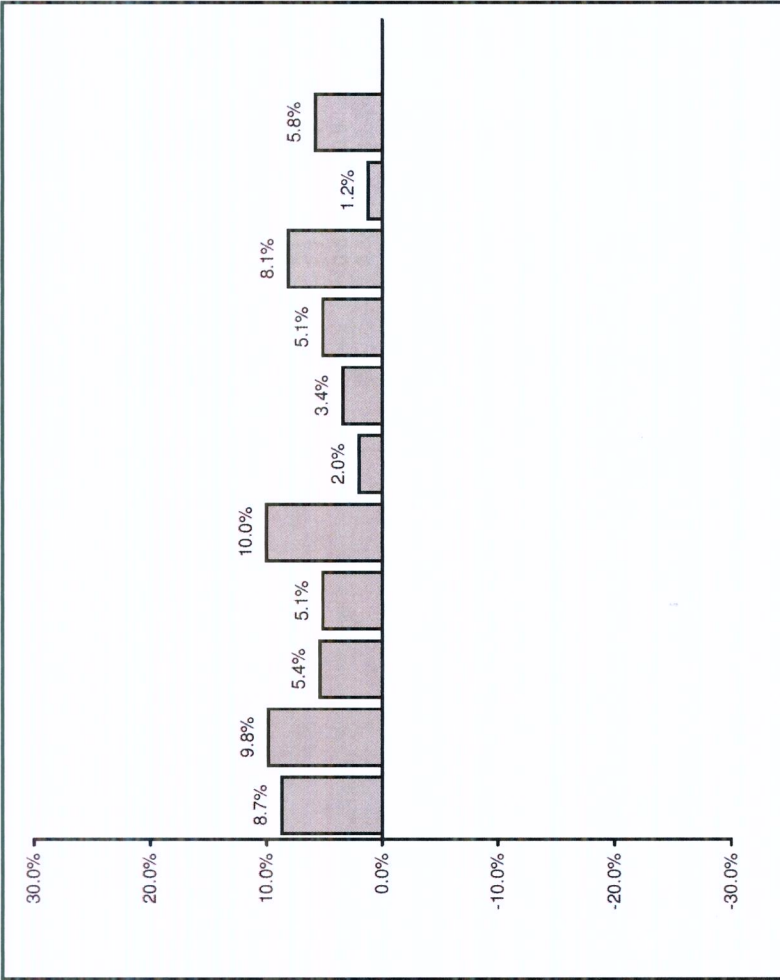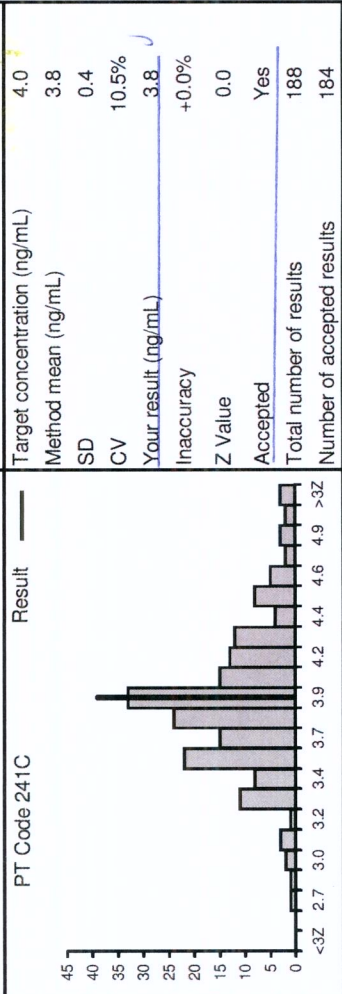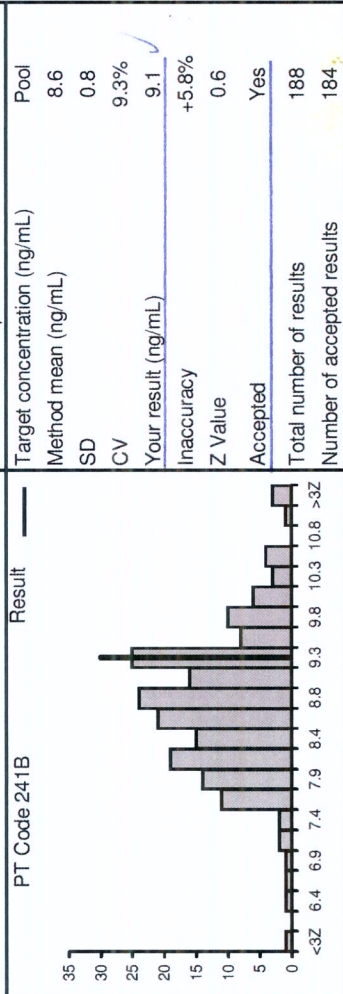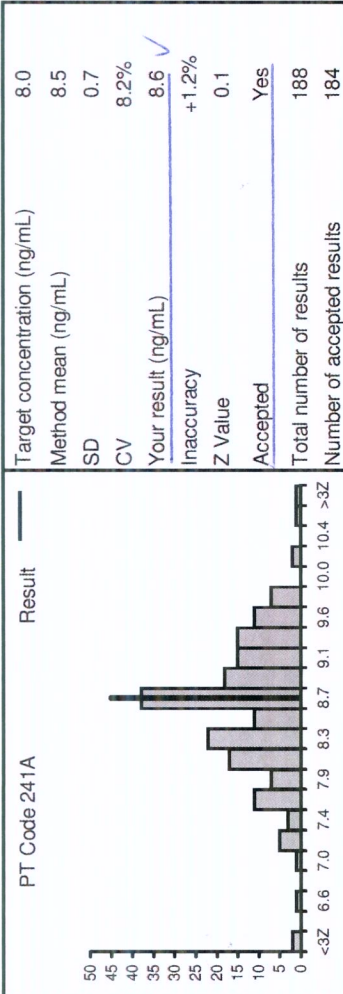

Target value	Pool	Pool	Pool	Pool	Pool	Pool	Pool	Pool	Pool	Pool	Pool	Pool
Method Mean	9.2	9.2	9.2	3.9	23.1	4.9	8.7	3.9	14.9	8.5	8.6	3.8
Your value	10.0	10.1	9.7	4.1	25.4	5.0	9.0	4.1	16.1	8.6	9.1	3.8
Accepted	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes